

Volumat™ Line

/L ST02-0

REF M46441960

Standard Infusion set

For use with Agilia VP MC pumps / Volumat MC Agilia pump or gravity only

With 1 roller clamp, 1 SafeClip (blue anti-free flow clamp), 1 pinch clamp, 1 proximal needle-free port, 1 rotating male luer lock and 1 flow stop cap. Does not contain natural rubber latex.

Inner diameter: ~0.118" (3 mm) Outer diameter: ~0.161" (4.1 mm)
















20

20 drops / mL approx

Do not use if package is damaged

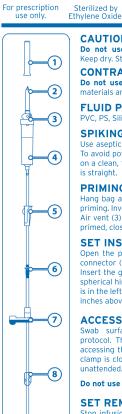

Do not use if package is damaged and/or protection caps are detached. Check set integrity. Keep dry. Store at controlled room temperature. Keep away from sunlight.

CONTRAINDICATIONS:

Do not use for light sensitive drugs and epidural. Some drugs may be incompatible with tubing materials and components: check drug labeling and hospital protocols.

FLUID PATH MATERIAL:

PVC, PS, Silicone, MABS, PC, Nontoxic, non-pyrogenic fluid path.

SPIKING TECHNIQUE:

Use aseptic technique. Close roller clamp (5). Remove cap (1) from spike (2). Insert spike into bag. To avoid potentially puncturing the solution bag with the spike, it is recommended to place the bag on a clean, flat surface, and/or spike the bag while holding by the inlet port to ensure the inlet port

PRIMING (before connecting to patient):

Hang bag and fill drip chamber (4) to approximately 1/2 full. Slowly open the roller clamp (5) for priming. Invert needle-free port (9) while priming and gently tap valve to remove all air and prime set. Air vent (3) should remain in a closed position unless infusing from a rigid bottle. When set is fully primed, close roller clamp (5), and check carefully for the absence of air bubbles.

SET INSTALLATION IN PUMP:

Open the pump door by lifting the door lever. Align the tubing set horizontally with the green connector (6) positioned to the right and the SafeClip (7) positioned in front of the clamp guide. Insert the green connector (6) in the green slot. Position the SafeClip (7) in the blue slot with the spherical hinge in the top position. Push the SafeClip (7) into the clamp guide. Ensure that the tube is in the left tube guide, then push the door lever to close the pump door. Hang the container 8 to 32 inches above the pump. Before turning on the pump, check the complete infusion setup.

ACCESS TO NEEDLE-FREE PORTS:

Swab surface prior to and after every use according to CDC guidelines or hospital protocol. The proximal needle-free port (9) may be used to administer a manual bolus; when accessing the needle-free port (9), we recommend that the infusion is stopped and the proximal clamp is closed (8). We also recommend luer lock connections only. If using luer slip, do not leave

Do not use sharp needle or blunt cannula with the needle-free port.

SET REMOVAL FROM PUMP:

Stop infusion. Close roller clamp (5), open door, remove infusion set from pump. Disconnect the set from IV access and container in accordance with hospital protocol. Set should not be used for more than 96 hours or 10 liters infusion, replace per hospital protocol or CDC guidelines. Discard biohazardous waste according to hospital protocol.

For Gravity use, ensure roller clamp (5) is closed, then open SafeClip (7) as shown below. Flow rate is regulated by roller clamp (5). Ensure roller clamp wheel moves freely when roller clamp (5) is in full open position.



Closed position after using in Pump.



Opened position (allows flow and gravity use)



(11)

FRESENIUS KABI

Manufactured by Fresenius Kabi AG 61346 Bad Homburg Germany

Imported and distributed in USA by: Fresenius Kabi USA, LLC Three Corporate Drive Lake Zurich, Illinois 60047

www.fresenius-kabi.us



(01)04250273714272 (17)YYMMDD (10)XXXXXXXX



YYYY-MM-DD



YYYY-MM-DD

expiration date



XXXXXXX

Made in XXXXXX

Imported and distributed in Canada by: Fresenius Kahi Canada Ltd

165 Galaxy Blvd, Suite 100 Toronto, ON M9W 0C8 www.fresenius-kabi.ca

(Les renseignements français sont disponibles sur demande.)